



检测报告 (Test Report)

No. BOLQHZZQ495717L1

样品名称 (Sample Description)	一次性使用医用口罩 Disposable Medical Face Mask
委托单位 (Applicant)	武汉友福国际贸易有限公司 Wuhan Youfu International Trade Co.,Ltd

PONY 谱尼测试
Pony Testing International Group
www.ponytest.com



检测结果

(Test Results)

No. BOLQHZZQ495717L1

第 1 页, 共 2 页 (page 1 of 2)

样品名称 (Sample Description)	一次性使用医用口罩 Disposable Medical Face Mask	样品规格 (Sample Specification)	规格 Specification: 17.5*9.5cm 型号 Model: 成人型 type of adult
委托单位 (Applicant)	武汉友福国际贸易有限公司 Wuhan Youfu International Trade Co.,Ltd	商标 (Trade Mark)	——
到样日期 (Received Date)	2020-11-02	生产日期或批号 (Manufacturing Date or Lot No.)	生产日期 Manufacturing Date: 2020 年 08 月 26 日 August 26,2020 生产批号 Manufacturing Lot No.: 20200826
检测日期 (Test Date)	2020-11-02~2020-11-13	样品等级 (Sample Grade)	——
样品数量 (Sample Quantity)	100 个 100pcs	检测类别 (Test Type)	委托检测 (Commissioning Test)
样品状态 (Sample Status)	正常 Normal	检测环境 (Test Environment)	符合要求 (To meet the requirements)
样品来源 (Sample Source)	送样 Send Sample		
检测项目 (Test Items)	见下页 See the next page		
检测方法 (Test Methods)	见下页 See the next page		
所用主要仪器 (Main Instruments)	电热恒温培养箱 Electric Heating Constant Temperature Incubator、 细菌过滤效率检测仪 Bacterial filtration efficiency detector 等 etc.		
检测结论 (Test Conclusion)	该样品经检测, 所检项目符合 EN 14683: 2019+AC: 2019 IIR 型的要求。 The sample has been tested and the tested items meet the requirements of EN 14683: 2019+AC: 2019 Type IIR.		
备注 (Note)	限值标准 Limit Standard: EN 14683: 2019+AC: 2019 生产单位Manufacturer: 武汉友福国际贸易有限公司Wuhan Youfu International Trade Co.,Ltd 受检单位Inspection: 武汉友福国际贸易有限公司Wuhan Youfu International Trade Co.,Ltd 以上样品信息由委托单位提供 The information of above sample was provided by the applicant.		
	编制人 (Edited by)	黄斌	
	审核人 (Checked by)	徐静	
	批准人 (Approved by)	戴晴	
	签发日期 (Issued Date)	2020-11-13	


检测结果 (Test Results)

No. BOLQHZZQ495717L1

第 2 页, 共 2 页 (page 2 of 2)

样品名称和编号 (Sample Description and Number)	检测项目 (Test Items)	限值 (Limit)	检测结果 (Test Results)		单项结论 (Evaluation)	检测方法 (Test Methods)
		IIR 型 Type IIR				
Q495717L1 一次性使用医用 口罩 Disposable Medical Face Mask	细菌过滤效率 (BFE), % Bacterial filtration efficiency(BFE)	≥98	No.1	>99.9	符合 Conform	EN 14683: 2019 +AC: 2019
			No.2	>99.9		
			No.3	>99.9		
			No.4	>99.9		
			No.5	>99.9		
	压力差, Pa/cm ² Differential pressure	<60	48.5		符合 Conform	EN 14683: 2019 +AC: 2019
	抗溅压力, kPa Splash resistance pressure	≥16.0	>16.0		符合 Conform	EN 14683: 2019 +AC: 2019
	微生物清洁度, cfu/g Microbial cleanliness	≤30	<1		符合 Conform	EN 14683: 2019 +AC: 2019

样品编号和照片 (Sample Number and Photo):

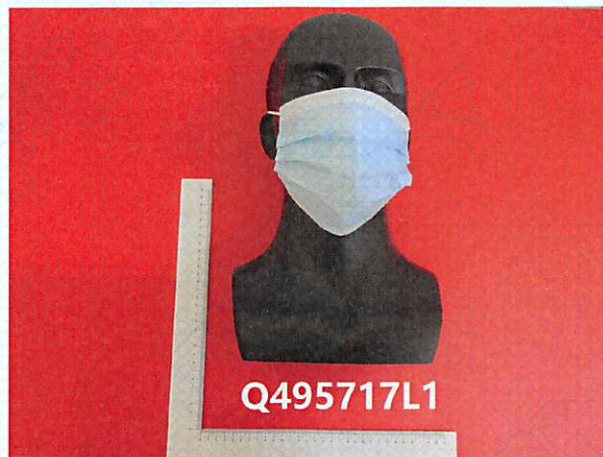

仅对报告照片中的样品负责

Pony authenticate the photo on original report only

——以下空白——

(End of Report)

TEST REPORT

(Electronic version)

扫码下载报告

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: XLBH-4640-24



No: 200342194

ISSUE DATE: 2020-11-09

APPLICANT: WUHAN YOUFU INTERNATIONAL TRADE CO., LTD
ADDRESS: ROOM3, 18/F, BUILDING S-1, KAILEGUIYUAN, NO.108, ZHUODAOQUAN ROAD, HONGSHAN DISTRICT, WUHAN CITY, HUBEI PROVINCE

INFORMATION CONFIRMED BY APPLICANT:
DISPOSABLE FACE MASK (NON MEDICAL USE)
QUANTITY: 100 PIECES

STANDARD ADOPTED:
T/CNTAC 55-2020, T/CNITA 09104-2020 <Civil sanitary mask>

DATE RECEIVED/DATE TEST STARTED: 2020-11-02

CONCLUSION:

BACTERIAL FILTRATION EFFICIENCY	M
PARTICLE FILTRATION EFFICIENCY	M
AIRFLOW RESISTANCE	M
BREAKING STRENGTH OF JUNCTION BETWEEN MASK STRING AND MASK BODY	M

NOTE: "M" - MEET THE STANDARD'S REQUIREMENT "F" - FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" - NO COMMENT

REMARK:
THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200342193.
THE DECISION INDICATORS ARE DERIVED FROM THE GROUP STANDARD REQUIRED BY CLIENT
(T/CNTAC 55-2020, T/CNITA 09104-2020). OUR INSPECTION CAPACITY AUTHORIZED BY CMA COVERS THE INSPECTION ITEMS
T/CNTAC 55-2020, T/CNITA 09104-2020.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

Yuan Liu ENGINEER

刘 圆



PAGE 1 OF 3

TEST REPORT

(Electronic version)

No:200342194



TEST REPORT

(Electronic version)

No:200342194

BACTERIAL FILTRATION EFFICIENCY (%)

M

(YY 0469-2011 ANNEX B, TEST BACTERIA: STAPHYLOCOCCUS AUREUS ATCC 6538, TEST AREA: 49cm², FLOW RATE: 28.3L/min, MEAN PARTICLE SIZE: 3.0 μm, RESULT OF THE POSITIVE CONTROL: 1.9×10³ CFU, RESULT OF THE NEGATIVE CONTROL: <1CFU)

REQUIREMENT

BFE₁ 99.3

≥95

BFE₂ 99.2

(T/CNTAC 55-2020, T/CNITA 09104-2020)

BFE₃ 99.2

PARTICLE FILTRATION EFFICIENCY (%)

M

(YY 0469-2011 5.6.2, AIR FLOW: 30L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION: 15mg/m³, TEMP: 21.9℃, RH: 38.6%)

REQUIREMENT

MINIMUM 96.42

≥90

(T/CNTAC 55-2020, T/CNITA 09104-2020)

AIRFLOW RESISTANCE (Pa)

M

(YY 0469-2011 5.6.2, AIR FLOW: 30L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION: 15mg/m³, TEMP: 21.9℃, RH: 38.6%)

REQUIREMENT

MAXIMUM 47.9

≤49

(T/CNTAC 55-2020, T/CNITA 09104-2020)

BREAKING STRENGTH OF JUNCTION BETWEEN MASK STRING AND MASK BODY (N)

M

(GB/T 13773.2-2008)

(GB/T 13773.2-2008 idt ISO 13935-2:1999)

REQUIREMENT

10

≥5

(T/CNTAC 55-2020, T/CNITA 09104-2020)



——End of Report——

PAGE 3 OF 3